

Abstract

This paper presents the preliminary results of nocturnal Aerosol Optical Depth (τ_a) and Angström Exponent (α) obtained from a new lunar photometer prototype, trade name Cimel CE-318U. Due to the variation of the moon's illumination inherent to the lunar cycle, the typical Langley-plot Method used in solar photometry to calibrate these instruments cannot be applied. In this paper we propose three different methods to carry out the lunar-photometer calibration. In order to validate the results we have selected three events, which encompass seven nights and ten days under different atmospheric conditions, including several saharan dust intrusions episodes. Method#1 is introduced in this work as a modification of the usual Langley Method. This technique, called Lunar-Langley Method, requires the extraterrestrial irradiances from a lunar irradiance model, providing similar accuracies on τ_a to those of AERONET (± 0.01 – 0.02). It makes comparable daytime and nighttime measurements. Method#2 consists of transferring the current calibration from a master used by sunphotometers. Its results are again within the limit of accuracy expected for the instrument. Method#3 uses an integrating sphere and the methodology proposed by Li et al. (2008) to determine sky calibration coefficients (C_j) and the instrument's solid angle field-of-view (Ω), respectively. We observe significant τ_a differences between Method#1 and #3 (up to 0.07), which might be attributed to the errors propagation in Method#3. The good results obtained from the comparison against a second CE-318U prototype, and against daytime data from a precision filter radiometer, constitute a valuable assessment of CE-318U performance. Results of α and its spectral variation ($\delta\alpha$) show good agreement between daytime and nighttime, being able to identify the aerosol properties associated with each event.

1 Introduction

Atmospheric aerosols are known to impact the climate evolution but they still represent one of the largest uncertainties in climate change studies (IPCC, 2007). The high

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



uncertainty associated to the role played by aerosols in radiative forcing on a global scale makes it necessary to obtain a global ground-based aerosol climatology. In this sense, the Aerosol Robotic Network (AERONET) is nowadays one of the most powerful worldwide tool (Holben et al., 1998). Aerosol Optical Depth (τ_a) at a certain wavelength is the standard parameter measured by sunphotometers such as those operating in AERONET. Spectral dependence of τ_a is mainly driven by the scattering efficiency and can be expressed by means of the classical Angström's equation (Angström, 1929). In the solar spectrum, the Angström exponent (α) is a good indicator of the dominant size of the atmospheric particles. τ_a and α data obtained from AERONET stations are used to provide independent and trustable validation to satellite-based aerosols products and to regional and global aerosol/dust models. However the lack of nighttime aerosol observations introduces some uncertainties in column aerosol estimations. Nighttime τ_a is a necessary parameter to derive a continuous sequence of total column aerosol information which is of considerable importance for monitoring aerosol transport, for high latitude locations, given the extended periods of darkness during winter, to study the effect of aerosol particles on cloud lifetime and coverage during the night, and for detecting massive aerosol outbreaks at night (Zhang et al., 2008).

Ground or spaceborne lidar observations have the capability to detect atmospheric column aerosols at night. However, its spatial coverage is limited and the τ_a observations can no longer constrain the extinction solution from the backscattering observations (Zhang et al., 2008). Passive sensors for τ_a measurements at night must solve the problem of the low incoming energy from the nocturnal celestial bodies, which emit in a range of 10^{-5} – 10^{-6} the sun's energy in the case of the moon, and five orders of magnitude less for the brightest star in the sky, Sirius. Stellar photometers are proven to be more effective in determining τ_a at nighttime than lunar photometers, but due to the low-income energy from the stars, the complexity of the large-aperture instrumentation limits their use and their implementation in standardized regional or global networks.

On the contrary, the relatively high irradiance from the moon provides the possibility of using common-aperture photometers to retrieve aerosol properties at night.

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Nevertheless the moon can be considered a solar diffuser with an exceptional stability, although the apparent brightness of this celestial body changes continuously with the lunar viewing geometry, such as the lunar phase or the libration angles, and due to the non-lambertian reflectance properties of its surface. These elements present important complexities and limitations in determining the instrument calibration. This problem was tackled by Berkoff et al. (2011) by considering a lunar irradiance model which explicitly accounts for the effects of phase, the spatial variegation of the lunar surface, the changes in the hemisphere of the moon presented to an observer (the lunar librations) and the strong backscatter enhancement at low phase angles (the so-called “opposition effect”) (Kieffer and Stone, 2005). This empirical model, known as ROLO (RObotic Lunar Observatory), was developed at the United States Geological Survey (USGS) as a NASA-funded project in support of the Earth Observing System (EOS) program. ROLO enables using the moon as a radiometric calibration source for on-orbit calibration of Earth observing satellites by means of a lunar spectral irradiance model that was developed from extensive telescopic observations acquired over more than 8 yr (Kieffer and Stone, 2005). Kieffer and Stone (2005) found band-average residuals less than 1 % by fitting thousands of ROLO observations at wavelengths from 350 to 2450 nm. Consequently, the model provides the exo-atmospheric lunar spectral irradiance with high precision for any given location and time within the model’s valid geometric range of phase angles ± 90 degrees. Berkoff et al. (2011) combined this information with nocturnal photometric measurements using a classical Cimel CE-318 sunphotometer to obtain atmospheric columnar multi-wavelength τ_a values. They studied this magnitude for two different atmospheric conditions near full-moon, and used a sunphotometer that was limited by a non-ideal laboratory based calibration. However, their results showed relatively low differences between observed τ_a values and those retrieved by close-in-time AERONET observations in the case of low and stable τ_a conditions. For the high and non-stable τ_a period, this study showed higher uncertainties in τ_a , especially in shorter-wavelength bands, resulting from the dark noise limit of the post-photodiode electronics. Moreover, these authors proposed the improvement of the

photo detector signal-to-noise ratio in order to use this type of photometers during the bright half of lunar phase and over much wider range of wavelengths and conditions. Concerning problems derived from calibration uncertainties, they can be partially fixed with a mountain-top Langley calibration or collocating stellar reference measurements.

5 In this study we have used two prototypes of a new instrument developed by Cimel Electronique for lunar photometry, trade name CE-318U photometer, specifically designed to track the moon and to perform automatic lunar irradiance measurements. These instruments were installed at the high mountain Izaña Observatory (2400 m a.s.l.) in order to characterize their performance, to obtain absolute calibrations and to
10 develop a reliable and trustable validation against reference instruments. We examined τ_a and α retrievals under very different nocturnal atmospheric conditions, including saharan dust intrusions with high τ_a , during a relatively long period, and compared them with daytime observations.

This paper starts with a brief description of the experimental site and its facilities (Sect. 2). In Sect. 3 the CE-318U instrument is briefly described as well as the main
15 spectral and temporal characteristics of the lunar measurements. In Sect. 4 we detail the methodology to obtain τ_a and α , which requires an ad-hoc calibration procedure in case of lunar observations. Three methods have been used to assess the instrument calibration: the Lunar-Langley Method, the calibration transference from a master, and
20 the calibration using an integrating sphere, which are presented in Sect. 5. The main results of this study are summarized in Sect. 6, where we analyze and compare lunar τ_a obtained by means the Lunar-Langley and our ROLO model implementation, showing some case analysis. We also compared τ_a and α obtained during night period with
25 daytime τ_a and α . Finally, the main conclusions of this work are presented in Sect. 7.

2 Site information

The high mountain Izaña Observatory, managed by the Izaña Atmospheric Research Centre (IARC), from the State Meteorological Agency of Spain (AEMET) is located in

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Tenerife (Canary Islands, Spain; 28° 18' N, 16° 29' W, 2363 m a.s.l.). This observatory is most of the time representative of free troposphere conditions, mainly in the night period where a downward catabatic regime is well established, providing excellent conditions for accurate measurements of trace gases. A strong temperature inversion layer normally located between 800 and 1500 m a.s.l., below the Izaña level, prevents the arrival of local or regional pollution from lower levels at the Observatory. This Observatory is part of the World Meteorological Organization (WMO) Global Atmospheric Watch Programme (GAW) and part of the Network for the Detection of Atmospheric Composition Change (NDACC). Furthermore, Izaña is a suitable place for sky observations due to a high atmospheric stability, high frequency of pristine days, a low and stable total column ozone and a very dry atmosphere. Several radiometric techniques, such as FTIR (Fourier Transform Infrared spectrometry), UV (i.e. Brewer spectrophotometers), DOAS (Differential Optical Absorption Spectroscopy) and Lidar have been used for a long time.

For our purposes it is worthy to highlight that Izaña Observatory is a direct-sun calibration site of AERONET (<http://aeronet.gsfc.nasa.gov>) and for its associated networks PHOTONS (PHOtometrie pour le Traitement Operationnel de Normalisation Satellitaire; <http://loaphotons.univ-lille1.fr/photons/>) and RIMA (Red Ibérica de Medida fotométrica de Aerosoles; <http://www.rima.uva.es>). In fact, PHOTONS, RIMA and IARC forms the present AERONET-Europe calibration infrastructure within the European project ACTRIS (Aerosols, Clouds, and Trace gases Research InfraStructure Network; <http://www.actris.net>), and Izaña Observatory is the site where master sunphotometers of AERONET-Europe are sun-calibrated. Izaña Observatory is part of the GAW Precision Filter Radiometer (PFR) network, managed by the World Radiation Center (Davos; Switzerland), whose mission is to obtain high accuracy long term τ_a and α series. Finally, Izaña Observatory hosts the reference triad of the WMO-GAW Regional Brewer Calibration Center for Europe (RBCC-E) (<http://www.rbcc-e.org>).

3 Instrumentation

3.1 The new lunar Cimel CE-318U

The new lunar Cimel CE-318U photometer is, in essence, a similar instrument to the classical sunphotometer Cimel CE-318, extensively described in Holben et al. (1998), but with new improvements and features introduced to allow the retrieval of the reduced incoming energy from the moon. This new instrument performs nocturnal measurements with high gain and an approximate field of view of 1.29° at eight nominal wavelengths of 1640, 1020, 938, 937, 870, 675, 500 and 440 nm. A sequence of three measurements is taken every 30 s at each wavelength. These triplets allow us to detect and screen clouds in the same way that they are used in sun-photometry. A new moon tracker has been built in the system. It is based in a four-quadrant detector with new electronics to amplify the signal, incorporating a new software to process data while tracking. This new tracker is also able to track the sun with a special device containing an attenuation filter to reduce the high incoming energy.

CE-318U combines the features of the standard Cimel sunphotometers with a rather good signal-to-noise ratio. We have calculated the instrument's stability by means of a triplet stability checking in case of diurnal and nocturnal measurements. As in sun photometry, each triplet value is defined as the maximum minus minimum divided by the mean value of the three consecutive measurements taken every 30 s. Results are presented in Table 1. Triplets values are wavelength dependent, and, in case of nocturnal measurements, they are also dependent on the moon's phase. They are appreciably lower for direct-sun measurements, especially in shorter wavelength channels, where the variability in triplets is the highest. This implies that daytime measurements are more stable than nocturnal ones, although the stability in daytime and near full moon observations is quite similar.

We have used two prototypes of the new CE-318U since July 2011. The most stable was considered as the master instrument, hereinafter referred to as CE-1, and the second prototype as the secondary instrument, hereinafter referred to as CE-2.

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

In this study we have included three different case studies. The first one involves a period of five consecutive nights in August (from 9 to 14) 2011, affected by different dust intrusions. The second one is a relatively low τ_a case study during 11 and 12 October 2011, while the third one is a very low and constant τ_a event during 8 to 9 February 2012.

3.2 The integrating sphere for radiances calibration

A calibration system developed for the instruments performing sky radiance measurements within the AERONET-PHOTONS-RIMA networks has been implemented at the Izaña Observatory. In such systems, the light source comes from an integrating sphere providing a homogeneous visual field. The recalibration of the sphere is accomplished three times a year by comparison to the travel NASA master Cimel sunphotometer (Guirado et al., 2012). Following Walker et al. (1991), the sphere's precision is assumed $\leq 5\%$.

3.3 ROLO model

In this paper, we have used the model presented in Kieffer and Stone (2005) to calculate the lunar irradiance (ROLO model) using our own astronomical calculations. ROLO Project was established to characterize the brightness of the moon with the aim of addressing the critical calibration problems of the Earth remote-sensing imaging sensors (Kieffer and Stone, 2005). This program was developed at the USGS Flagstaff Science Center in Arizona as a NASA-funded project. The basis of this program is the automated ground-based observations over multiple years to capture the cyclic brightness variation of the moon. The observatory was in operation for more than 8 yr, observing every clear night at lunar phases within $\pm 90^\circ$. Over 85 000 lunar images were acquired in 32 wavelengths from 350 to 2450 nm. These images form the basis data for the model, as spatially integrated lunar irradiance measurements. The ROLO model uses

an empirically derived analytic equation to predict the lunar disk-equivalent reflectance (A_j) in the spectral band j using only geometric variables (Kieffer and Stone, 2005),

$$\ln(A_j) = \sum_{n=1}^3 a_{i,j} g^n + \sum_{n=1}^3 b_{n,j} \varphi^{2n-1} + c_1 \cdot \theta + c_2 \cdot \phi + c_3 \cdot \varphi \cdot \theta + c_4 \cdot \varphi \cdot \phi + d_{1,j} \cdot e^{-\frac{g}{\rho_1}} + d_{2,j} \cdot e^{-\frac{g}{\rho_2}} + d_{3,j} \cdot \cos\left(\frac{g - \rho_3}{\rho_4}\right) \quad (1)$$

where g is the absolute phase angle, θ and ϕ are the selenographic latitude and longitude of the observer, respectively, and φ is the selenographic longitude of the sun.

Kieffer and Stone (2005) found band-average absolute residuals about 1 % by comparison between ROLO empirical irradiances and hundreds of ROLO observations. Consequently, ROLO provides the exo-atmospheric lunar irradiance with a relatively high precision over the full range of the geometric variables and wavelengths at a specific location and time. Since our modeled irradiances were computed using a different astronomical ephemeris calculator and for the actual viewing geometry, a lower level of accuracy in our ROLO-implemented model is expected. The ephemeris used in this study is the Alcyone ephemeris 4.3, based on the Moshier's ephemeris and the celestial mechanics equations from Meeus (1991), both adjusted to the Jet Propulsion Laboratory's DE404 results. It has an expected precision within 0.5'' in moon's longitude, 0.33'' in latitude and 0.36 km in distance.

3.4 Ancillary information for data validation

τ_a and α obtained with the Izaña AERONET instrument (<http://aeronet.gsfc.nasa.gov>), near sunset and near sunrise, are used to compare with τ_a and α determined with CE-1 and CE-2 at moonrise and moonset, respectively.

A 4-wavelength GAW precision filter radiometer (PFR) developed by the World Optical Depth Research and Calibration Center (WORCC) of the PMOD World Radiation Center (<http://www.pmodwrc.ch/worcc/index.html>) is in operation at Izaña since July

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



2001. PFR near sunset and near sunrise τ_a at 412.1, 501.0, and 863.1 nm, as well as α , were used as an additional reference to validate the CE1 and CE-2 data.

A Micropulse Lidar (MPL), MPL-3 (SES Inc., USA) system (Spinhirne et al., 1995) has been running at Santa Cruz de Tenerife station (28.5° N, 16.2° W; 52 m a.s.l.) since 5 January 2005. This program has been implemented for monitoring and characterization of Saharan Air Layer (SAL) North Atlantic outflow, and it is currently in operation within NASA/MPLNET (<http://mplnet.gsfc.nasa.gov>), and is co-managed by National Institute for Aerospace Technology (INTA; Spain) and the Izaña Atmospheric Research Centre (IARC; AEMET). MPL is a robust system with high-pulse frequency (2500 Hz) and low-energy (7–10 μ J, maximal) “eye-safe” Nd:YLF laser at 523 nm operational in full-time 10 continuous mode (24 h a day/365 days a year). Lidar backscattered signal is registered in 1-min integrated time and with a vertical resolution of 75 m. Details of the MPL and the on-site maintenance and calibration techniques are described by Campbell et al. (2002). It is used to track the SAL dust layering structure evolution from day to day, 15 and be compared qualitatively with τ_a evolution obtained with AERONET and lunar photometers. In this study we have processed lidar data and obtained backscatter cross sections.

FLEXible backward TRAjectories (FLEXTRA) plots from the EMPA facility for Global 20 GAW stations have been used to confirm the pathways of air masses arriving to Izaña at several levels. The calculations are based on the FLEXTRA model and driven by ECMWF wind fields with a global resolution of 1° × 1°. FLEXTRA trajectory images are available at <http://lagrange.empa.ch/>.

A new method for nocturnal aerosol measurementsA. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



4 Methodology

4.1 Aerosol optical depth determination – the Lunar-Langley method

Attenuation of moon's irradiance in an atmospheric window, as occurs during daytime, can be described by the Beer-Lambert-Bouguer Law:

$$V_{\lambda} = V_{0,\lambda} \cdot \exp(-m(\theta) \cdot \tau_{\lambda}) \quad (2)$$

where V_{λ} is the output voltage, $V_{0,\lambda}$ represents the extraterrestrial voltage, which includes all temporal variations (lunar phase as well as earth-moon and moon-sun distances), m is the relative optical mass, function of the moon's zenith angle θ , and τ_{λ} is the spectral optical depth. For the air-mass and the spectral optical depth calculation we have followed the specifications given by Holben et al. (1998). Moon's zenith angle (θ) has been obtained using the ephemeris Alcyone 4.3. Taking logarithms on both sides of Eq. (2) we have,

$$\ln(V_{\lambda}) = \ln(V_{0,\lambda}) - m(\theta) \cdot \tau_{\lambda} \quad (3)$$

To account for the change in moon's illumination during the course of the night as well as the distance effect on lunar irradiance, we have introduced in Eq. (2) these the two contributions on the V_0 term. Thus,

$$V_{0,j} = I_{0,j} \cdot \kappa_j \quad (4)$$

where $I_{0,j}$ is the extraterrestrial irradiance in a certain channel with a central wavelength at j , and κ_j is a constant that depends on the instrument features. $I_{0,j}$ is calculated using the ROLO lunar disk-equivalent reflectances (A_j) in Eq. (1). It takes into account lunar phase as well as sun-moon distance. In this work, the sun-moon distance as well as the selenographic latitude and longitude of the observer and the sun are computed using the astronomical calculator previously described. Lunar reflectances are converted to modeled irradiances using the following expression,

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



$$I_j = \frac{A_j \cdot \Omega_M \cdot E_j}{\pi} \quad (5)$$

In this equation Ω_M is the moon's solid angle, dependent on the moon-earth distance and E_j is the solar spectral irradiance for the band j . Following Kieffer and Stone (2005), to obtain the last term the irradiance model of Wehrli (1986) has been assumed,

$$E_j = \frac{\int_{\lambda_1}^{\lambda_2} E_s(\lambda) \cdot R(\lambda) d\lambda}{\int_{\lambda_1}^{\lambda_2} R(\lambda) d\lambda} \quad (6)$$

where $E_s(\lambda)$ is the sun's spectral irradiance at 1 AU and $R(\lambda)$ is filter response function for each spectral band of CE-318U. Regarding Ω_M , it is obtained using the topocentric apparent diameter of the moon (d_{app}), function of earth-moon distance,

$$\Omega_M = \pi \cdot \left(\sin \frac{d_{app}}{2} \right)^2 \quad (7)$$

With all these inputs on the Eqs. (1) and (5) moon's irradiance was calculated coincidentally with each CE-318U measurement.

The calibration methodology for nocturnal photometry proposed here for nighttime measurements is called Lunar-Langley Method. It uses Eqs. (3) and (4) and a least squares fitting to obtain the instrument's calibration constant (κ_j) as the intercept of the fitting line. In this case κ_j constants strictly accounts for the instrument's photometric responsivity and any residual systematic offset difference between ROLO predicted $I_{0,j}$ and the actual exoatmospheric irradiance. Thus, it must be ideally computed as an average of some Lunar-Langley's obtained in a mountain-top station under suitable atmospheric conditions.

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



As in daytime period, a good Lunar-Langley calibration requires clean, cloud-free and stable atmospheric conditions. For this reason it is commonly applied in sun-photometry over a range of air masses between 2 and 5 during sunrise or sunset. In this study we have used the Lunar-Langley methodology to obtain the calibration constants κ_j 's under stable and clear atmospheric measurements, over a range of air masses between 2 and 5 (during the moonrise or the moonset).

Once κ_j 's are known by means of the Lunar-Langley Method, it is possible to determine instantaneous τ_a from an individual measurement:

$$\tau_{a,j} = \frac{\ln\left(\frac{V_j}{I_{0,j}}\right) - \ln(\kappa_j) - m_{\text{atm}}(\theta) \cdot \tau_{\text{atm},j}}{m_a(\theta)} \quad (8)$$

The subscript “atm” accounts for air mass and optical depth of each atmospheric attenuator with the exception of aerosols.

4.2 Angström's exponent (α) determination

The spectral dependence in τ_a can be used as an indicator of the aerosol's scattering efficiency. This dependence is usually expressed by means of the Angström exponent (α) derived from the Angström Law (Angström, 1929). α is a qualitative indicator of aerosol particle size or fine mode fraction (Kaufman et al., 1994). Thus, the combined α - τ_a information is useful to discriminate the different aerosol types.

To obtain this parameter we have retrieved τ_a within the spectral range between 870 nm and 440 nm. Taking the slope of the linear fit to the logarithm of λ_j vs. logarithm of $\tau_a(\lambda_j)$ ($j = 870, 675, 500$ and 440 nm channels), we can obtain α using the following equation:

$$\ln(\tau_a(\lambda_j)) = \ln(\beta) - \alpha \cdot \ln(\lambda_j) \quad (9)$$

Another important parameter is the spectral variation of α ($\delta\alpha$). It reports additional information about the aerosol size distribution, and it is expressed as,

$$\delta\alpha = \alpha(440, 675) - \alpha(675, 870) \quad (10)$$

Following Kaufman et al. (1993), negative values of $\delta\alpha$ indicate the dominance of only one mode of fine aerosols and positives values the coexistence of two separate particle modes. Basart et al. (2009) demonstrated that relatively small negative values indicate presence of pure mineral dust.

4.3 Instrument solid angle field-of-view determination

The solid angle field-of-view (solid angle FOV or Ω) of a photometer is normally provided by the manufacturer. However, in this work we have calculated it following the methodology proposed by Li et al. (2008). It computes Ω from daytime measurements using the aureole calibration coefficients (C_a) and instrument user and internal gains, instead of computing them by means of the classical laboratory method. The C_a coefficients are obtained by means of a calibration using an integrating sphere. These authors obtained from error propagation expected uncertainties between 3 % and 5 %. They propose the following definition for Ω :

$$\Omega = \Omega_g \cdot \frac{LG}{HG_a} = \left(\frac{E_0}{V_{0,s} \cdot C_a} \right) \cdot \frac{LG}{HG_a} \quad (11)$$

where Ω_g is the solid angle gain corrected, LG and HG_a are the direct and aureole instrument internal electronic gains, respectively, E_0 is the extraterrestrial solar irradiance, $V_{0,s}$ is the solar extraterrestrial constant and C_a are the aureole radiance calibration coefficients, obtained using the integrating-sphere calibration technique.

Results of Ω_j are shown in Table 2, showing a spectral dependence on this magnitude. This slight wavelength dependence was also found by Li et al. (2008), although they propose to average the spectral Ω_j over all wavelengths to derive a constant value.

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



5 Calibration strategy

As for sunphotometers, lunar-photometers need a calibration procedure in order to obtain τ_a and α , and to assess their reliability and intercomparability. Sunphotometer's calibration usually needs the estimation of the voltage measured by the instrument in absence of atmosphere by extrapolation of the voltage curve in Eq. (2) to zero air mass conditions. This calibration procedure is known as Langley-plot method. It uses the sun or, as in this case, the moon as a reference light source. However, this methodology must be re-formulated to account for the moon's irradiance variation inherent to the lunar cycle.

In this paper we present the calibration strategy for the lunar CE-318U instrument, which can be approached by three different methods, depending on available calibration facilities.

5.1 Method#1: "Lunar-Langley" calibration

The first method implies the determination of the calibration constants κ_j by means of the Lunar-Langley Method expressed by using the Eqs. (3) and (4). This Method requires the knowledge of the moon's extraterrestrial irradiance at any time of measurement. Once raw data and I_0 's are ratioed, the calibration constants κ_j can be determined as the intercept of the least squares fitting in Eq. (3).

We have performed this calibration technique for both CE-1 and CE-2 using the lunar data obtained on 8–9 February 2012. This night was selected due to the relatively low and constant τ_a conditions, especially during moonset, where τ_a at 440 nm remained stable and near 0.02. For CE-1, this calibration was applied in other two time periods to check the stability of the calibration.

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



5.2 Method#2: calibration transference from a master

The previous calibration method is very accurate, if suitable atmospheric conditions exist. For this reason, it can only be applied in mountain-top sites where very low and stable τ_a exists, as well as low humidity nighttime conditions can be attained. Only a few sites can meet these requirements, so an alternative calibration method is needed. The second proposed method is that followed by classical sunphotometers by means of intercomparisons. It is based on the calibration transference from a master instrument (Toledano et al., 2011), in turn calibrated at a high mountain site. This transference technique is possible taking into account the average ratio in digital counts between coincident measurements from two lunar photometers. Being $(\overline{DC_M})$ and $(\overline{DC_i})$ the average coincident raw data for the master and the instrument “i” to be calibrated, respectively, we can obtain the calibration constant $V_{0,i}$ using the known value $V_{0,M}$ obtained from a master, with the following expression:

$$V_{0,i} = V_{0,M} \cdot \frac{\overline{DC_i}}{\overline{DC_M}} \quad (12)$$

5.3 Method#3: calibration using an integrating sphere

A third method to calibrate a lunar photometer is based on the use of an integrating sphere to determine the sky calibration coefficients C_j , as Berkoff et al. (2011) followed, and the laboratory procedure developed by Li et al. (2008) to calculate Ω_j . The instrument coefficient's κ_j can be determined as follows,

$$\kappa_j = \frac{1}{C_j \cdot \Omega_j} \quad (13)$$

From Eqs. (4) and (13) we can determine experimentally the calibration coefficients for our instrument (κ_j 's) deriving C_j and Ω_j . Then, it could be possible to convert at any

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



time ROLO exo-atmospheric irradiances into the instrument V_0 parameter. $V_{0,j}$ inferred using this method has an accuracy strongly limited by the uncertainties involved in the determination of C_j and Ω_j , as well as those involved in the ROLO model.

In this study, we have used an integrating sphere calibration system implemented for PHOTONS-RIMA calibration at IARC. The main features of the integrating-sphere were described in Sect. 3.2.

6 Results

6.1 Method#1

The calibration constants k_j 's were calculated using this Lunar-Langley calibration for the two CE-318U prototypes using nocturnal measurements on the moonset of 9 February 2012 for CE-1, and the moonrise for CE-2, as no data was available for CE-2 during the moonset. This was the most pristine and stable event to perform an accurate Langley calibration. The coefficients of the two instruments are shown in Table 3.

Using the calibration coefficients from this table, nocturnal τ_a for CE-1 have been calculated for 9–10, 10–11, 11–12, 12–13 and 13–14 August 2011 and for two episodes more on 11–12 October 2011 and 8–9 February 2012, with low and stable aerosol conditions. In Figs. 1, 2 and 3 the daytime and nocturnal τ_a evolution is presented for a sequence of six days and five nights of measurements in August and the nights in October and February. Lidar backscatter vertical cross-section is shown in addition to the τ_a course for each episode in order to have independent qualitative information about the vertical structure and variability of the aerosols. For a quantitative analysis of daytime and nocturnal τ_a differences, it is necessary to establish a criterion of “quasi-simultaneity”. In this study we have compared nocturnal and daytime data corresponding to the consecutive 1-h time period during sunset–moonrise (SS–MR) and moonset–sunrise (MS–SR): the first hour of the moonrise against the last hour of previous daytime data during sunset, as well as the last hour of the moonset against

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



the first hour of subsequent daytime τ_a during sunrise. These results are shown in Table 4.

6.1.1 High τ_a conditions: saharan dust events

We used the information from FLEXTRA backward trajectories in order to infer dust source regions in the high τ_a events assigned to August 2011. They show air mass pathways over the Sahara and the Sahel in several height levels above Izaña Observatory up to 5500 m a.s.l. from 9 to 14 August (not shown here for the sake of brevity). These saharan dust intrusions during 9 and 10 August are clearly seen in Fig. 1. The first event is detected by the MPL with a maximum backscatter signal between 2 and 4 km height from 9 August to 10 August midday. After this time the signal decreases sharply, with minimum values at night. During this period some high clouds are detected by MPL at a height above 8 km, and thus, τ_a can be affected. Differences during moonrise and sunset on 9 August are below 0.01 (Table 4), within the τ_a accuracy limit established in AERONET (Holben et al., 1998). Nocturnal data was not available to perform moonset and sunrise comparison on 10 August. In the same day, these differences reached 0.02 in 440 nm during the moonrise, meanwhile they were reduced to values below 0.01 in the next moonset-sunrise period, when another intrusion started on 11 August. From 05:00 to 23:00 UTC, approximately, and after this period the backscatter signal decreased slowly. This change in aerosol concentration was well captured by CE-1, with a τ_a decreasing from values up to 0.20 in 440 nm during the early night to lower than 0.10 in 440 nm, and near constant values during the latest part of this night. From Table 4 we can see that sunset-moonrise and moonset-sunrise τ_a differences are similar, below 0.02 for all channels. We had a third intrusion in this period, on 13 August. In this case, the aerosol layer extended between near surface and 4 km altitude, starting at about 22:00 UTC. The dust layer is perfectly captured by the lidar profile and compares quite well to the aerosol optical depth curves obtained with CE-1. Nocturnal τ_a differences during the 12–13 August reached 0.02 for sunset-moonrise and 0.03 for moonset-sunrise in shorter wavelengths channels.

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



During the moonset and sunrise of 14 August differences grew to 0.04, due to the sharp τ_a increase. Meanwhile, in the sunset-moonrise of 13 August, just when this intrusion starts, τ_a differences are about 0.01. Although most of the differences found were higher than the AERONET accuracy limit for τ_a , they are explained by the high aerosol variability.

6.1.2 Low τ_a conditions

In order to test the performance of this new instrument over low and stable aerosol concentrations we have included two additional events. The first clean event showed a τ_a relatively constant (around 0.07 at 440 nm) test case during two consecutive days (11 and 12 October 2011), shown in Fig. 2. This figure demonstrates a good agreement between vertical aerosol backscatter evolution and τ_a , as well as between AERONET and CE-1 τ_a values. In Table 4, τ_a differences are ≤ 0.01 during both sunset-moonrise and moonset-sunrise. Although the increment in aerosol concentration during nighttime is well captured by CE-1, it can be seen from Fig. 2 a probable calibration problem affecting the 1640 nm and 1020 nm channels between moonrise and moonset.

The second clean event was on 8–9 February 2012 (Fig. 3). This is a very clear night (τ_a at 440 between 0.02 and 0.04) with a relatively stable aerosol concentration during the entire night, especially over the moonset period. On 9 February a Lunar-Langley was performed. In this case, as expected, moonset data matches pretty well AERONET sunrise data. Differences are slightly greater during moonrise but within the AERONET τ_a accuracy limit.

τ_a validation has been completed with daytime τ_a from PFR for 11 and 12 October 2011 and 8 and 9 February 2012. We should note that PFR has only three channels centered at 863.1, 501 and 412.1 nm. Therefore, the comparison study can only be computed for the CE-1 near coincident channels. AERONET versus PFR, as well as AERONET versus CE-1 τ_a differences are presented in Table 5. τ_a differences in quasi-simultaneous AERONET and CE-1 τ_a measurements are ≤ 0.02 for all channels in October, and below 0.01 in February, similar to the differences found between simultaneous

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



reference AERONET-PFR measurements, with values up to 0.017. These results confirm the optimum performance of the CE-1 under low τ_a conditions.

Regarding nocturnal τ_a from the CE-2, τ_a differences between AERONET and CE-2 are shown in Table 6. The agreement between these two references is pretty good, within the expected accuracy of ± 0.01 for longer wavelengths and ± 0.02 for shorter wavelengths. Since comparisons of both CE-1 and CE-2 show τ_a deviations within the expected limit of ± 0.01 , it indicates the robustness of this calibration method.

6.2 Method#2

τ_a results using Method#2 have been evaluated for 9 and 10 February 2012. This method is based on Eq. (12) for coincident measurements with a master (CE-1) and a secondary instrument (CE-2). In our case CE-2 was calibrated using the average ratio of raw data of the two instruments during a stable and clear night period. In this sense, 9 February 2012, was the best option, with a mean background τ_a (440 nm) ~ 0.02 .

The τ_a scatter-plot obtained using CE-1 and CE-2 is shown in Fig. 4. The τ_a differences and corresponding root-mean-square error (RMSE) are presented in Table 7. τ_a comparison for the day after the calibration (10 February) shows a good concordance between the values obtained from the master and the secondary instrument, with averaged differences up to 0.002.

6.3 Method#3

The third method for a lunar photometer calibration involves the determination of the sky calibration coefficients (C_j) using the integrating sphere procedure described in Sect. 3.2. The coefficients obtained for CE-1 using this Method are presented in Table 8. For comparison with Method#1, we have derived the CE-1 sky calibration coefficients (C_j'') from the κ_j coefficients in Table 3 considering the solid-angle Ω_j in Table 2. These C_j'' are also presented in Table 8. Comparing these coefficients we note that

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



those centered at 500 and 440 nm present higher relative differences, with values up to 0.25. Differences in the rest of channels are below 0.10. Higher discrepancies in shorter wavelengths channels might be due to uncertainties in the integrating sphere calibration technique because in these channels the sphere's radiant flux is notably reduced.

The averaged differences between τ_a obtained with the calibration coefficients calculated with this method (C_j) and those determined with Method#1 (C_j'') for 9–14 August 2011, 11–12 October 2011, and 8–9 February 2012 are shown in Table 9. Lower discrepancies are observed in channels 1020, 675 and 870 nm. However, only differences in 1020 nm are within the limit of instrumental precision of ± 0.01 –0.02. Discrepancies are significantly higher for the rest of channels, up to 0.07 for 500 nm central wavelength channel.

The previous results highlight the lower accuracy showed by Method#3, below the precision required to make comparable daytime and nighttime measurements. These discrepancies might be caused by a sum of contributions: (1) the accuracy on $I_{0,j}$ due to the implementation of the ROLO model (with an expected systematic error $\varepsilon \geq 0.01$); (2) the calibration errors from the integrated sphere method to obtain C_j 's ($\varepsilon = 0.03$ –0.05); and (3) uncertainties associated to the determination of the solid angle Ω ($\varepsilon = 0.03$ –0.05). Since the first contribution also affects to Method#1, it is necessary to increase the precision of the integrating sphere calibration as well as in the determination of Ω to improve the results in Method #3.

To check the error on the last contribution we have used the solid angle value provided by the manufacturer ($\Omega_{\text{ref}} = 3.4 \times 10^{-4}$ sr) and the coefficients C_j presented in Table 8. Ω_{ref} is the wavelength independent solid angle assumed by Berkoff et al. (2011) to obtain nocturnal τ_a information. A new τ_a comparison between Method#1 and #3 using Ω_{ref} is presented in Table 10. It can be seen that differences obtained are notably higher than those from table 9 for 1020 and 675 nm channels, slightly higher for 870 nm, similar for 1640 nm, slightly lower for 440 nm and considerably lower for 500 nm. These differences are higher than those reported by Berkoff et al. (2011). It

might indicate that the actual solid angle used by Berkoff et al. (2011) was closer to the manufacturer's reported value. These discrepancies clearly indicate that τ_a calculation is very sensitive to the methodology to estimate Ω .

6.4 Angström's exponent

5 Angström values have been obtained with CE-1 for the same cases analysis as for τ_a (11–14 August 2011, 11–12 October 2011, and 8–9 February 2012).

Nocturnal α values for CE-1 are computed as the slope of the linear regression of $\ln(\tau_a)$ versus $\ln(\lambda)$ using channels at 870, 675, 500 and 440 nm, as shown in Eq. (9). Mean daytime α values were extracted from AERONET database. Results for τ_a at
10 440 nm, α and $\delta\alpha$ are presented in Table 11 for the August 2011 case study, and in Table 12 for 11–12 October event. In these tables we have included the aerosol information extracted for the sunset (SS) and the moonrise (MR) as the average of the last 1-h data measured during daytime and nighttime, respectively. Moreover, we have considered data corresponding to sunrise (SR) and moonrise (MR), as the first 1-h
15 data of each day and night.

α data derived in the two case studies range from 0.1 to 1.2. The prevalence of low α values indicate the presence of large particles ($> 1\mu\text{m}$) during the saharan dust outbreaks. Minimum values below 0.2 are obtained for the periods 9–10 and 13–14 August, which coincide with two important saharan dust intrusions over Tenerife and
20 a maximum $\tau_a > 0.4$ (9 August). According to Basart et al. (2009), $\alpha = 0.6$ represents an appropriate threshold value of dust laden air masses influenced by other aerosols, while $\alpha \leq 0.3$ indicates the presence of pure desert dust. On the other hand, $\alpha > 0.7$ are found in those days with relatively low dust concentrations ($\tau_a < 0.10$) during the October case study, suggesting the presence of other aerosols. A good concordance
25 between daytime and nocturnal α values is found.

Finally, regarding the averages of the spectral variation of alpha ($\delta\alpha$) presented in Tables 11 and 12, we have obtained near zero or slightly negative $\delta\alpha$ values between -0.01 and 0.01 during the important dust intrusions starting on 11 August and 14

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



August. These results are consistent with the experimental values between -0.3 and 0.1 obtained by Basart et al. (2009) in case of coarse mode saharan aerosols. A stable period of $\delta\alpha$ between 0.2 and 0.3 was observed from moonset 11 August to moonrise 12 August, and from moonset 12 August to moonrise 13 August. For the October event, higher values are retrieved, between 0.3 and 0.4 . Positive values indicate the co-existence of two separate particle modes. It usually occurs when fine fraction aerosols appear well-mixed with coarse mode aerosols (Basart et al., 2009).

7 Summary and conclusions

In this paper we have described the preliminary results obtained with the new lunar photometer CE-318U, specifically designed to perform nocturnal photometric measurements. We have presented a first calibration strategy for this instrument which encompasses three different methods. Basically, this strategy requires the determination of the CE-318U calibration coefficients or their transference from a master instrument. The first Method consists of the adaptation of the usual Langley-plot method to nocturnal measurements. It introduces significant modifications to the current methodology, incorporating a lunar irradiance model (ROLO) to determine the instrument calibration coefficients. This strategy has been tested and validated using two CE-318U prototypes (CE-1 and CE-2), reporting discrepancies within the limit of τ_a accuracy of the instrument (± 0.01 – 0.02). For CE-1, this calibration was applied in other time periods, demonstrating the stability of the calibration. Moreover, nocturnal and daytime τ_a comparison using AERONET and PFR under low and stable τ_a conditions on 12 October 2011, showed similar differences between AERONET/PFR, AERONET/CE-1 and PFR/CE-1, within the AERONET τ_a accuracy. This comparison, against two independent reference instruments constitutes a valuable assessment of CE-318U performance.

Method#2 consists of transferring the calibration coefficients from a master. Results showed very close τ_a between the two lunar photometers, with differences below 0.01 .

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Method#3 is based on obtaining the sky calibration coefficients (C_j 's) using an integrating-sphere and then retrieving the calibration coefficients κ_j 's once the solid angle Ω is calculated. The comparison between τ_a obtained using Method#3 and the Method#1 shows significant τ_a differences of 0.07 and 0.05 for 500 and 1064 nm channels, respectively. For the rest of channels differences are lower, below 0.05, but higher than the limit of instrumental precision expected for this instrument (± 0.01 – 0.02). Such high discrepancies might be caused by the sum of errors in τ_a determination process using Method#3: (1) moon irradiances from ROLO model; (2) integrated sphere method to derive C_j 's; and (3) the methodology to calculate Ω . Our study highlights the importance of accounting for a high-performance integrating sphere and an accurate determination of Ω to assure a good calibration following Method#3.

Finally, the comparison between daytime and nocturnal α showed a good agreement between daytime and nighttime data. $\delta\alpha$ results are also in agreement with the expected values for different atmospheric conditions presented each night according to reference values reported in the literature.

The consistency of these results points to the capabilities of this new photometer to obtain aerosol properties at night. Since column aerosol optical properties are limited to the light period, this information becomes an important limitation in polar regions. In addition, monitoring the diurnal variation of aerosols is important in many sites associated to sea-land breezes, mountain-valley regime or the diurnal variations of the boundary layer height. It is also important for detecting the sharp changes that dust intrusions may experience in term of hours. Some sites with particular climatology present frequent clouds in the morning, while clear skies occurs during the night, resulting in important observation periods reduction with classical sunphotometers. Nowadays, lidar techniques, as those used in MPLNET, operate in full-time continuous mode (24 h a day/365 days a year) to detect qualitatively the atmospheric aerosol content and its vertical distribution. However, it is necessary to improve the lidar extinction-to-backscatter ratio using additional τ_a information provided by lunar-photometers during nighttime. τ_a and α determination during the night can be used for long-term and near

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



real time aerosol/dust models validation, as well as for new satellite-borne sensors verification. For example, the EUMETSAT Infrared Atmospheric Sounding Interferometer (IASI) sensor provides τ_a during the night (Klüser et al., 2012). So, validation of both model and satellite τ_a could be expanded to night periods. Concerning operational aerosol observations, the last eruption of the Volcano Eyjafjöll, in spring 2010, highlighted the weakness of the current monitoring of this type of aerosols and the importance of having a continuous observation system to support the aircraft navigation. The joint observations of lidar/ceilometers and lunar photometers at night could help to fill monitoring gaps existing today.

To conclude, CE-318U lunar photometers in operational networks could be used as complementary instruments to expand the column aerosol observation periods and to enhance the operational capability in the Aerosol Robotic Network (AERONET). However, the complexities inherent to the lunar irradiance pattern, make lunar photometry a difficult task compared to sun-photometry. Thus, despite the good results reported in this paper, it is necessary to design a more refined calibration procedure. Further developments should be oriented to develop a photometer capable of taking measurement during both daytime and nighttime. Concerning calibration, efforts should be paid to transfer direct-sun Langley calibration to moon observations.

Nevertheless, at the present state, lunar photometry is an attractive option to complete aerosol databases.

Acknowledgements. The authors wish to thank Cimel for providing the two prototypes used in this study as well as all the technical support. In addition, we wish to express special thanks to Mr. Stone, at the United States Geological Service (USGS) for helping to implement the ROLO model and provide wise counsel to this paper. The Aeronet sunphotometer at Izaña has been calibrated within AERONET-EUROPE TNA supported by the European Community – Research Infrastructure Action under the FP7 “Capacities” specific programme for Integrating Activities, ACTRIS Grant Agreement no. 262254. The GAW-PFR network for AOD at GAW Global observatories has been implemented by the World Optical Depth Research and Calibration Center (WORCC). We want to thank Mr. Wehrli for supporting quality control and quality assurance of GAW-PFR data and for personal communications in this paper. Finally, the authors would like

to express their thanks to the security staff at Izaña Observatory for kindly supporting the night operation of the lunar instruments. The integrating sphere was provided by the Infrastructure project entitled “RIMA: instrumental para infraestructura de calibración fotométrica (RIMA-LC)”, Ref. UNVA05-23-038 from the Atmospheric Optics Group (GOA) at the University of Valladolid.

5 References

- Angström, A. K.: On the atmospheric transmission of sun radiation and on the dust in the air, *Geogr. Ann. A*, 12, 130–159, 1929. 5529, 5539
- Basart, S., Pérez, C., Cuevas, E., Baldasano, J. M., and Gobbi, G. P.: Aerosol characterization in Northern Africa, Northeastern Atlantic, Mediterranean Basin and Middle East from direct-sun AERONET observations, *Atmos. Chem. Phys.*, 9, 8265–8282, doi:10.5194/acp-9-8265-2009, 2009. 5540, 5548, 5549
- Berkoff, T. A., Sorokin, M., Stone, T., Eck, T. F., Hoff, R., Welton, E., and Holben, B.: Nocturnal aerosol optical depth measurements with a small-aperture automated photometer *J. Atmos. Ocean. Tech.*, 28, 1297–1306, doi:10.1175/JTECH-D-10-05036.1, 2011. 5530, 5542, 5547, 5548
- Campbell, J. R., Hlavka, D. L., Welton, E. J., Flynn, C. J., Turner, D. D., Spinhirne, J. D., Scott, V. S., and Hwang, I. H.: Full-time, eye-safe cloud and aerosol lidar observation at atmospheric radiation measurement program sites: instrument and data processing, *J. Atmos. Ocean. Tech.*, 19, 431–442, 2002. 5536
- Guirado, C., Ramos, R., de Frutos, Á., Berjón, A., Redondas, A., López, C., Cachorro, V., Cuevas, E., González, R., González, S., and Hernández, M.: Optical calibration facility at the Izaña atmospheric research center, *Opt. Pura Apl.*, 45, 57–62, 2012. 5534
- Holben, B. N., Eck, T. F., Slutsker, I., Tanré, D., Buis, J. P., Setzer, A., Vermote, E., Reagan, J. A., Kaufman, Y. J., Nakajima, T., Lavenu, F., Jankowiak, I., and Smirnov A.: AERONET – a federated instrument network and data archive for aerosol characterization, *Remote Sens. Environ.*, 66, 1–16, 1998. 5529, 5533, 5537, 5544
- IPCC – Intergovernmental panel on climate change: *Climate Change 2007: the Physical Science Basis*, Cambridge University Press, UK, 2007. 5528
- Kaufman, Y. J.: Aerosol optical thickness and atmospheric path radiance, *J. Geophys. Res.*, 98, 2677–2692, 1993. 5540

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- Kaufman, Y. J., Gitelson, A., Karnieli, A., Ganor, E., and Fraser, R. S.: Size distribution and phase function of aerosol particles retrieved from sky brightness measurements, *J. Geophys. Res.-Atmos.*, 99, 10331–10356, 1994. 5539
- 5 Kieffer, H. H. and Stone, T. C.: The spectral irradiance of the moon, *Astronomical J.*, 129, 2887–2901, 2005. 5530, 5534, 5535, 5538
- Klüser, L., Kleiber, P., Holzer-Popp, T., and Grassian, V. H.: Desert dust observation from space – application of measured mineral component infrared extinction spectra, *Atmos. Environ.*, 54, 419–427, 2012. 5551
- 10 Li, Z., Blarel, L., Podvin, T., Goloub, P., Buis, J. P., and Morel, J. P.: Transferring the calibration of direct solar irradiance to diffuse-sky radiance measurements for Cimel sun-sky radiometers, *Appl. Optics*, 47, 1368–1377, 2008. 5528, 5540, 5542
- Meeus, J.: *Astronomical Algorithms*, 1st edn., Willmann-Bell Inc., Richmond, Virginia, USA, 1991. 5535
- 15 Spinhirne, J. D., Rall, J. A. R., and Scott, V. S.: Compact eye safe lidar systems, *Rev. Laser Eng.*, 23, 112–118, 1995. 5536
- Toledano, C., Cachorro, V. E., Berjón, A., de Frutos, A. M., Fuertes, D., González, R., Torres, B., Rodrigo, R., Bennouna, Y., Martín, L., and Guirado, C.: RIMA-AERONET network: long-term monitoring of aerosol properties, *Opt. Pura Apl.*, 44, 629–633, 2011. 5542
- 20 Walker, J. H., Cromer, C. L., and McLean, J. T.: Calibration of passive remote observing optical and microwave instrumentation, in: *Proceedings Spie – the international soc. of optical engineering*, Vol. 1493, 3–5 April 1991, Orlando, FL, USA, 224–230, 1991. 5534
- Wehrli, C.: *Spectral Solar Irradiance Data*, WMO ITD 149, Geneva, 1986. 5538
- Zhang, J., Reid, J. S., Miller, S. D., and Turk, F. J.: Strategy for studying nocturnal aerosol optical depth using artificial lights, *Int. J. Remote Sens.*, 29, 4599–4613, 2008. 5529

A new method for nocturnal aerosol measurements

A. Barreto et al.

Table 1. CE-318U triplets in % obtained for two nights with different moon's fraction of illumination (FI) and for daytime measurements.

	Type of measurements	Channels (nm)					
		1020	1640	870	675	440	500
13 Dec 2011	Nocturnal (FI = 87 %)	0.36	0.18	0.23	0.26	0.61	0.52
9 Feb 2012	Nocturnal (FI = 93 %)	0.28	0.13	0.18	0.19	0.30	0.25
22 Dec 2011	Daytime	0.09	0.11	0.09	0.13	0.15	0.22

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 2. CE-1 solid angle (in steradians) determined with daytime measurements.

Channel (nm)	1020	1640	870	675	500	440
Ω_j	3.92×10^{-4}	3.95×10^{-4}	3.93×10^{-4}	3.88×10^{-4}	3.82×10^{-4}	3.78×10^{-4}

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 3. κ_j calibration constants extracted for each channel (in nm) for CE-1 and κ' coefficients for CE-2, both obtained on 9 February 2012 ($W^{-1} m^2 nmDC$).

Channel (nm)		1020	1640	870	675	500	440
CE-1 κ_j	mean	2.15×10^9	1.28×10^{10}	3.02×10^9	2.29×10^9	1.74×10^9	1.41×10^9
CE-2 κ_j'	mean	2.01×10^9	1.15×10^{10}	2.74×10^9	2.10×10^9	1.64×10^9	1.33×10^9

A new method for nocturnal aerosol measurements

A. Barreto et al.

Table 4. τ_a averaged differences between daytime AERONET and CE-1 data during sunset-moonrise (SS–MR, as the last 1 h of daytime AERONET data versus the first 1 h of nocturnal CE-1 data) and moonset-sunrise (MS–SR, as the first 1 h of daytime AERONET data versus the last 1 h of nocturnal CE-1 data).

	Channel (nm)	1020	1640	870	675	500	440
9–10 Aug. 2011	SS–MR	0.001	0.005	–0.003	0.011	–0.002	–0.006
	MS–SR	–	–	–	–	–	–
10–11 Aug 2011	SS–MR	–0.010	–0.001	–0.007	–0.008	–0.009	0.015
	MS–SR	0.015	0.008	0.005	0.006	0.004	–0.003
11–12 Aug 2011	SS–MR	–0.017	–0.007	–0.015	–0.015	–0.016	–0.017
	MS–SR	–0.012	–0.010	–0.013	–0.015	–0.018	–0.023
12–13 Aug 2011	SS–MR	–0.016	–0.009	–0.021	–0.021	–0.022	–0.019
	MS–SR	–0.019	–0.019	–0.023	–0.025	–0.028	–0.029
13–14 Aug 2011	SS–MR	–0.014	–0.009	–0.013	–0.013	–0.014	–0.013
	MS–SR	–0.024	–0.035	–0.032	–0.032	–0.031	–0.032
11–12 Oct 2011	SS–MR	0.002	0.007	0.008	0.006	0.007	0.005
	MS–SR	–0.007	–0.005	–0.003	–0.004	–0.002	–0.003
8–9 Feb 2012	SS–MR	–0.006	–0.009	–0.011	–0.014	–0.016	–0.015
	MS–SR	0.001	0.001	0.001	–0.002	–0.002	–0.003

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

Table 5. τ_a averaged differences on 11 to 12 October 2011 and 8 to 9 February 2012 between daytime PFR and nocturnal CE-1 data during sunset-moonrise (SS–MR, the last 1 h of daytime PFR data versus the first 1 h of nocturnal CE-1 data) and moonset-sunrise (MS–SR, as the first 1 h of daytime PFR data versus the last 1 h of nocturnal CE-1 data). τ_a differences between PFR and AERONET during moonrise and moonset have been included.

	PFR Channel (nm)	421.1	501	863.1
PFR/CE-1	Oct SS–MR	0.017	0.010	0.012
	Oct MS–SR	0.016	0.010	0.009
	Feb SS–MR	–0.006	–0.009	–0.008
	Feb MS–SR	0.005	0.004	0.001
PFR/AERONET	Oct SS–MR	–0.011	–0.006	–0.004
	Oct MS–SR	–0.017	–0.013	–0.012
	Feb SS–MR	–0.006	–0.004	–0.001
	Feb MS–SR	–0.007	–0.006	0.001

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 6. τ_a averaged differences between daytime AERONET and nocturnal CE-2 data for the same time period as in Tables 4 and 5 for 8–9 February 2012. Moonset-sunrise data was not available.

Channel (nm)	1020	1640	870	675	500	440
SS–MR	–0.005	–0.006	–0.007	–0.010	–0.013	–0.014

A new method for nocturnal aerosol measurements

A. Barreto et al.

Table 7. τ_a averaged differences (\bar{d}) and RMSE for nocturnal coincident measurements of two lunar photometers (CE-2 minus CE-1) on 9 and 10 February 2012.

	Channel (nm)	1020	1640	870	675	500	440
9 Feb	\bar{d}	0.001	0.002	0.001	0.001	0.003	0.001
	RMSE	0.001	0.002	0.001	0.001	0.003	0.001
10 Feb	\bar{d}	0.001	0.001	-0.001	-0.001	-0.001	-0.002
	RMSE	0.001	0.002	0.001	0.001	0.001	0.001

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


A new method for nocturnal aerosol measurements

A. Barreto et al.

Table 8. Master sky calibration coefficients C_j calculated using an integrating sphere and C_j'' obtained from κ_j 's and solid angles previously determined, both in $\text{W m}^{-2} \text{nm}^{-1} \text{DC}^{-1}$. The spectral relative variation between both coefficients (Δ_{rel}) is included.

Channel (nm)	1020	1640	870	675	500	440
CE-1 C_j	1.16×10^{-6}	2.15×10^{-7}	8.95×10^{-7}	1.15×10^{-6}	2.02×10^{-6}	1.70×10^{-6}
CE-1 C_j''	1.19×10^{-6}	1.97×10^{-7}	8.42×10^{-7}	1.13×10^{-6}	1.51×10^{-6}	1.88×10^{-6}
Δ_{rel}	0.02	0.08	0.06	0.03	0.25	-0.10

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


A new method for nocturnal aerosol measurements

A. Barreto et al.

Table 9. Averaged τ_a differences (\bar{d}) and RMSE for five-days nocturnal period (9–14 August 2011, 11–12 October 2011, and 9–10 February 2012) obtained with calibration Method#1 and #3 using CE-1 photometer data.

Channel (nm)	1020	1640	870	675	500	440
\bar{d}	−0.012	0.051	0.035	0.016	0.071	0.042
RMSE	0.013	0.053	0.037	0.017	0.074	0.044

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


A new method for nocturnal aerosol measurements

A. Barreto et al.

Table 10. Averaged τ_a differences (\bar{d}) and RMSE for five-days nocturnal period (10–14 August 2011, 11–12 October 2011, and 8–9 February 2012) obtained with calibration Method#3 and #1 using CE-1 photometer data. Solid angle was assumed as $\Omega_{\text{ref}} = 3.4 \times 10^{-4}$ sr, reported by the manufacturer.

Channel (nm)	1020	1640	870	675	500	440
\bar{d}	0.094	0.056	0.048	0.060	−0.004	0.019
RMSE	0.095	0.057	0.050	0.062	0.004	0.020

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Table 11. Averaged values of τ_a (in 440 channel), α (Angström exponent) and $\delta\alpha$ obtained in August, 2011, case study. Values are for SS (sunset), MR (moonrise), MS (moonset) and SR (sunrise).

		$\tau_{a,440}$	α	$\delta\alpha$
9 Aug	SS	0.41	0.19	0.04
	MR	0.40	0.16	0.04
10 Aug	MS	0.40	0.16	–
	SR	0.32	0.12	–0.03
	SS	0.12	0.35	0.04
11 Aug	MR	0.14	0.33	0.23
	MS	0.18	0.29	0.14
	SR	0.17	0.25	0.01
	SS	0.19	0.25	–0.01
12 Aug	MR	0.20	0.23	0.02
	MS	0.11	0.48	0.22
	SR	0.01	0.46	0.14
	SS	0.07	0.63	0.15
13 Aug	MR	0.09	0.44	0.08
	MS	0.09	0.56	0.17
	SR	0.06	0.68	0.20
	SS	0.07	0.63	0.16
14 Aug	MR	0.08	0.53	0.17
	MS	0.12	0.12	0.06
	SR	0.15	0.24	0.02
	SS	0.30	0.16	0.05

A new method for nocturnal aerosol measurements

A. Barreto et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

Table 12. Averaged τ_a in 440 nm, α and $\delta\alpha$ for 11–12 October 2011. Values are for SS (sunset), MR (moonrise), MS (moonset) and SR (sunrise).

	11–12 October			
	SS	MR	MS	SR
τ_a	0.07	0.07	0.07	0.06
α	1.03	1.19	0.91	1.08
$\delta\alpha$	0.40	0.25	0.23	0.47

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


A new method for nocturnal aerosol measurements

A. Barreto et al.

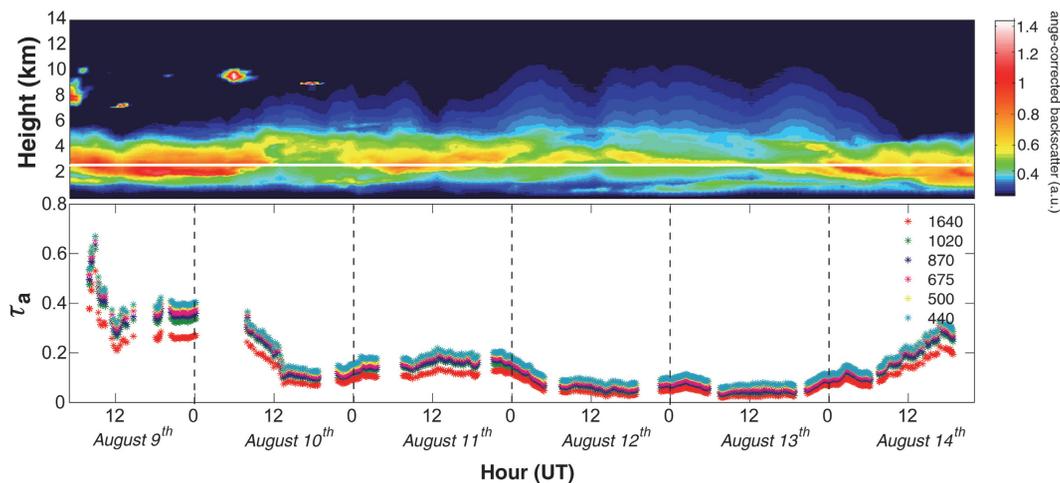


Fig. 1. τ_a evolution during six days and five nights on August, 2011, using AERONET data for daytime and lunar CE-1 data for nocturnal period. MPL corrected backscatter cross-sections obtained at Santa Cruz station in upper panel. The white line represents the Izaña Observatory level.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



A new method for nocturnal aerosol measurements

A. Barreto et al.

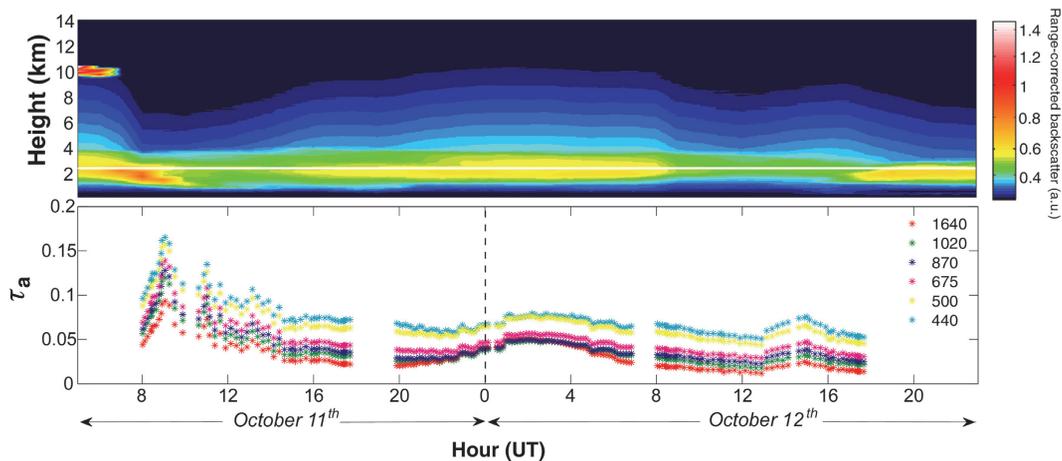


Fig. 2. CE-1 τ_a on 11 and 12 October 2011 with MPL corrected backscatter cross-sections for the same period (upper panel). The white line represents the Izaña Observatory level.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

A new method for nocturnal aerosol measurements

A. Barreto et al.

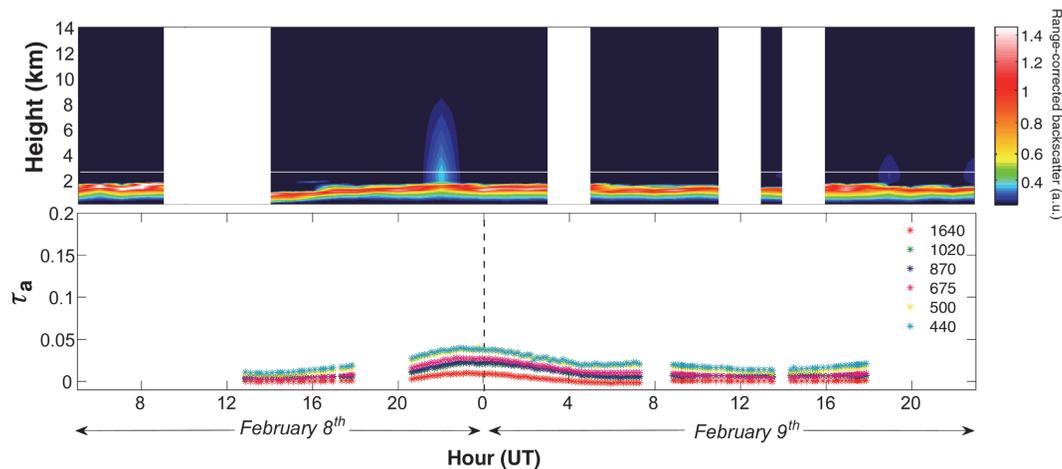


Fig. 3. CE-1 τ_a on 8 and 9 February 2012, with MPL corrected backscatter cross-sections. The white line represents the Izaña Observatory level.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

A new method for nocturnal aerosol measurements

A. Barreto et al.

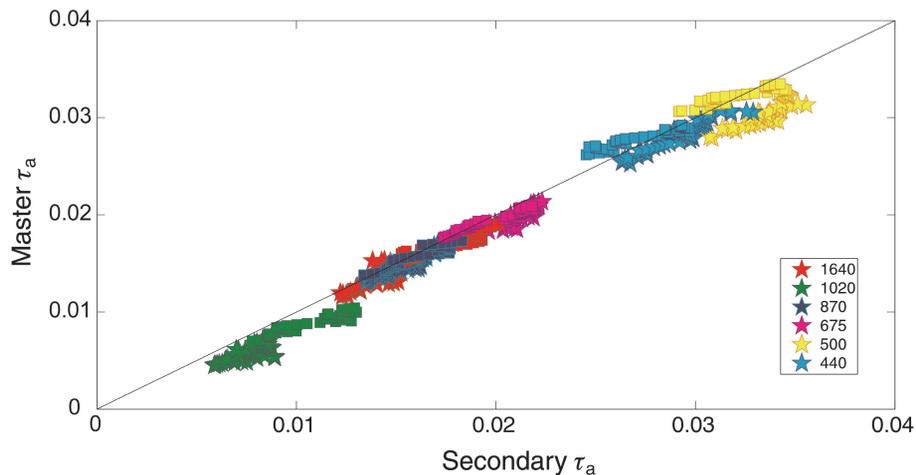


Fig. 4. τ_a scatter-plot obtained for CE-1 (master) and CE-2 (secondary) using calibration Method#2 for 9 February (stars) and 10 February (squares) 2012.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)